
Connection to Injector/Platform Device is Red?

Troubleshooting · https://dropletlab.com/knowledge-doc/what-to-do-if-the-connection-to-injector-platform-device-is-red/

In this case, verify that the injector/platform is connected to the power.

Click the Reconnect icon to reconnect the device.

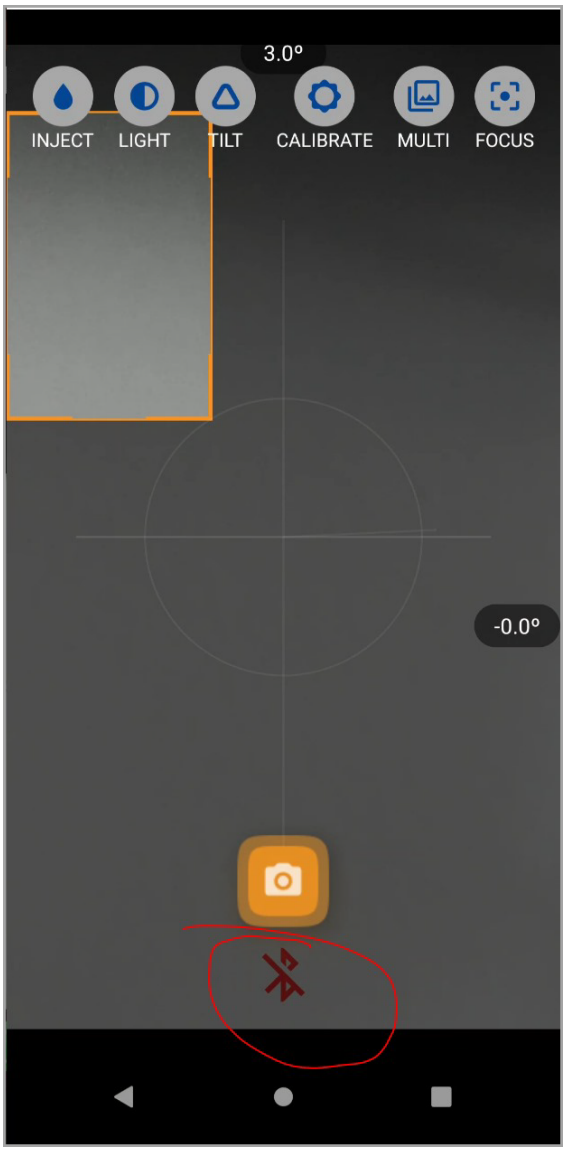

Restart the injection device.